

# MOS-200

Simple, Fast, Sensitive

Compatible with all SFM models




## Absorbance - Fluorescence 90° light scattering - Chemiluminescence

### Simple and optimized for kinetics

MOS-200 is an efficient single grating manual monochromator spectrometer. It has been specially designed to offer you the highest speed and sensitivity in rapid kinetics acquisitions. Coupled to one of our stopped-flow model it offers the most complete and flexible stopped-flow spectrometer configuration available.

A Xe(Hg) or Xe high intensity light source is used for illumination of sample. Connection to the stopped-flow cuvette is done through a fiber optic cable, which guarantees maximum and uniform light efficiency from the grating to the observation cell. Excitation wavelength is selected manually. Cut-off or low pass band filters can be used to select emission wavelength in fluorescence mode.


Bio-Kine is the reference software for kinetics studies. It includes efficient tools which provide fast and accurate data collection, display and analysis.

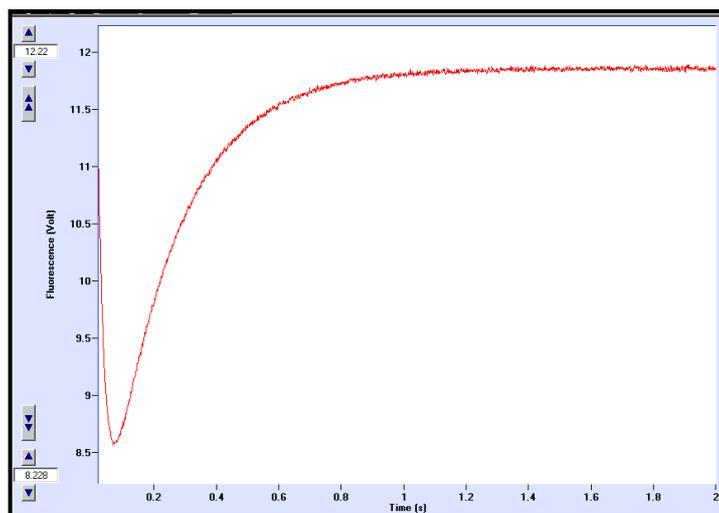

### Fast and sensitive


Detection is made using a high sensitivity photomultiplier tube (PMT) optimized for wavelength from 160 to 850 nm. **The same PMT can be used for both absorbance and fluorescence measurements: switch from one configuration to the other takes only 30 seconds !.**

The operator has the choice between single and multi time base acquisition modes with a **fastest sampling period of 1 measurement per 10 μs**. Combined with the **250 μs dead time** of the stopped-flow it offers ideal conditions for ultra-fast kinetics. Sampling rate is adjustable so complex reactions with different steps can be followed easily.

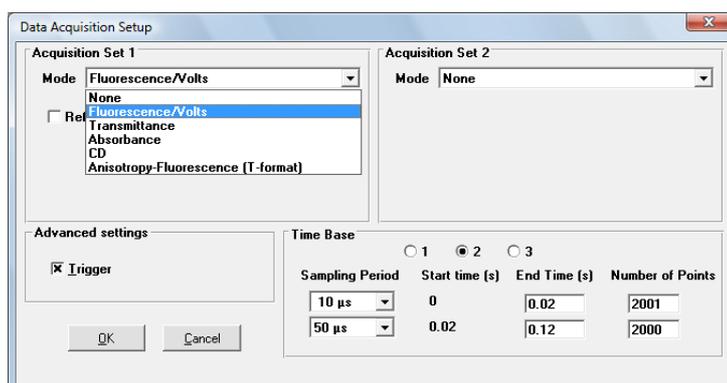

## User-friendly

**Bio-Kine includes analysis functions** so data can be fitted using predefined or user-defined equations. Operations such as smoothing, linear or Log sampling, and baseline subtractions are standard. RMS noise analysis is available, and residuals analysis helps you estimate the quality of the fit. Data is saved as text files for easy transfer to other software.

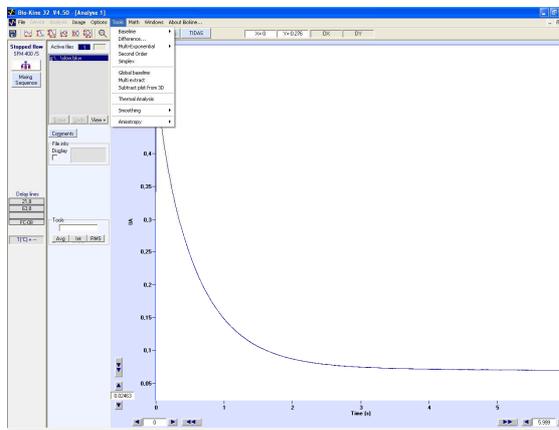

## Specifications

| Light source              |  |
|---------------------------|--|
| Number of lamps           | 2  |
| Nature/Power              | super quiet 150W Xe(Hg) <b>and</b> 150W Xe (tungsten lamp available in option) |
| Wavelength range          | 220 to 700 nm Xe(Hg)<br>200 to 800 nm Xe                                       |
| Stability                 | better than 1% for Xe(Hg)<br>better than 0,3% for Xe                           |
| Nature of spectrum        | sharp lines for Xe(Hg)<br>continuous spectrum for Xe                           |
| Light source power supply |  |
| Ripple ( 50 to 60Hz)      | < 0,1 % rms  |
| Low frequency noise       | < 0,05 % peak to peak  |
| Drift                     | < 0,1% minute after one hour warm up   |
| Manual Monochromator      |  |
| Grating                   | 1200 grooves/ nm   |
| Focal length              | 100 mm   |
| Aperture                  | F/# = 3,5  |
| Wavelength range          | zero order and 200-800 nm  |
| Linear dispersion         | 8 nm/mm  |
| Accuracy                  | ± 0,5 nm   |

*Specifications are subject to change without prior notice*

| Fiber optic                 |   |
|-----------------------------|---|
| Material                    | quartz  |
| Wavelength range            | 200-800 nm  |
| Length                      | 1,5 m   |
| Dimensions                  | 1mm x 3mm ( monochromator side)<br>1,9 mm diameter ( stopped-flow side) |
| Detection                   |   |
| Photomultiplier tube        | 11 stage, optimized for UV <b>and</b> visible                           |
| Operating voltage           | 0 to 1200 V   |
| Wavelength range            | 160 to 850 nm   |
| Low-pass filters            | manual  |
| Data acquisition            |   |
| Acquisition board type      | High speed 4 channel A/D  |
| Sampling rate               | 10 µs to 1000s/ point   |
| Number of time bases        | 1 to 3  |
| Noise level in fluorescence | S/N > 1000 at 1 ms integration time<br>(using FC-15 and 1µM NATA)       |
| Noise level in absorbance   | 5x10 <sup>-5</sup> AU rms at 1ms integration time                       |
| System requirements         | Windows PC with 2000, XP, Vista and<br>1 open PCI slot (required)       |

### Included with MOS-200

- ◆ Optical rail
- ◆ Manual monochromator
- ◆ Photomultiplier tube and control unit
- ◆ Photomultiplier control unit (PMS-250)
- ◆ Acquisition board and communication cable
- ◆ 320 nm cut-off filter
- ◆ Single light source + power supply (ALX-250)
- ◆ 1.5 meter fiber optics (other dimensions available on request)
- ◆ Fiber optics adaptor for stopped-flow head
- ◆ Trigger cable
- ◆ Biokine and SFit software
- ◆ Connector block (PCI / PMS-250 / Trigger)

## Endless upgrade possibilities

### Additional detection channel :

For simultaneous absorbance/fluorescence and double fluorescence measurements. This includes a second photomultiplier tube and control unit.

### T-format anisotropy kit :

It includes a set of Glan-Taylor polarizers and an additional detection channel. Polarizers are installed in PMT holder for easy removal in absorbance mode. Triple simultaneous measurements (absorbance/T-format anisotropy, fluorescence) is available with optional 049-10.

### Motorization of monochromator

For full software control of excitation wavelength and PMT voltage. It includes MM-450. It allows kinetics in wavelength tracking mode( multi wavelength measurements). Automatic reconstruction of 3D data for global fitting analysis

### MOS-200/M and MOS-450/AF-CD :

MOS-200 can be upgraded to higher spectrometer models to access detection techniques such as Circular Dichroism, Linear dichroism and Fluorescence Anisotropy using **our patented EMFA method (Excitation Modulated Fluorescence Anisotropy)**.

Bio-Logic, SAS  
1, rue de l'Europe  
38640 CLAIR - France  
Tel.: +33 476 98 68 31  
Fax: +33 476 98 69 09  
www.bio-logic.info



Bio-Logic USA, LLC  
P.O.Box 30009  
Knoxville TN 37930 - USA  
Tel.: +1 865 769 3800  
Fax: +1 865 769 3801  
Web: www.bio-logic.us

# MOS-200/M

The motorized version

Compatible with all SFM models




## Absorbance - Fluorescence 90° light scattering - Chemiluminescence

### Fast and sensitive

**MOS-200/M is the motorized version of MOS-200.** It offers the same speed and sensitivity with the addition of full software control over wavelength, PMT gain, and acquisition speed. Coupled to one of our stopped-flow model it offers the most complete and flexible stopped-flow spectrometer configuration available.

**A double Xe/Xe(Hg) light source** allows changing lamps without any lamp handling. It is perfect for easy switching from kinetics to steady state applications. Connection to the stopped-flow cuvette is done through a fiber optic cable, which guarantees maximum and uniform light efficiency from the grating to the observation cell. Cut-off or low pass band filters can be used to select emission wavelength in fluorescence mode.

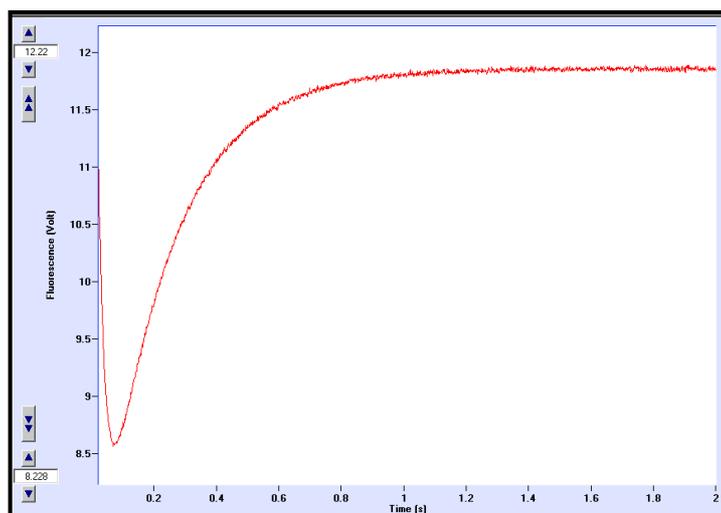


### Full automation

Detection is made using a high sensitivity photomultiplier tube (PMT) optimized for wavelength from 160 to 850 nm. **The same PMT can be used for both absorbance and fluorescence measurements: switch from one configuration to the other takes only 30 seconds !.** The PMT is fully software controlled.


The operator has the choice between single and multi time base acquisition modes with a **fastest sampling period of 1 measurement per 10 μs**. Combined with the **250 μs dead time** of the stopped-flow it offers ideal conditions for ultra-fast kinetics. Sampling rate is adjustable so complex reactions with different steps can be followed easily.

**Wavelength tracking mode** : the user can program a series of shots at different wavelength to build 3D data (λ, time, signal) . Such data give access to SVD and global fitting analysis using **Sfit** with a 10 μs resolution !

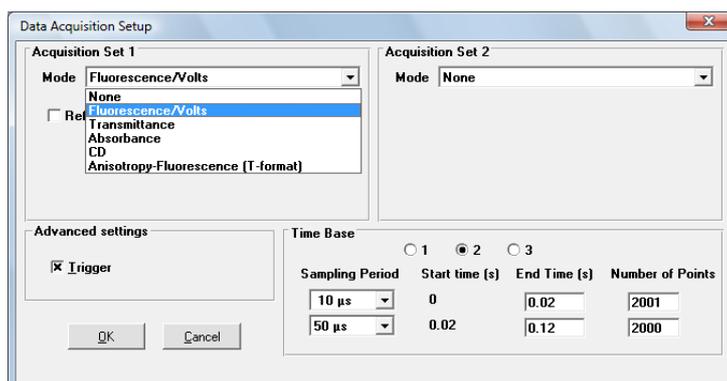

## User-friendly software

**Bio-Kine includes analysis functions** so data can be fitted using predefined or user-defined equations. Operations such as smoothing, linear or Log sampling, and baseline subtractions are standard. RMS noise analysis is available, and residuals analysis helps you estimate the quality of the fit. Data is saved as text files for easy transfer to other software.

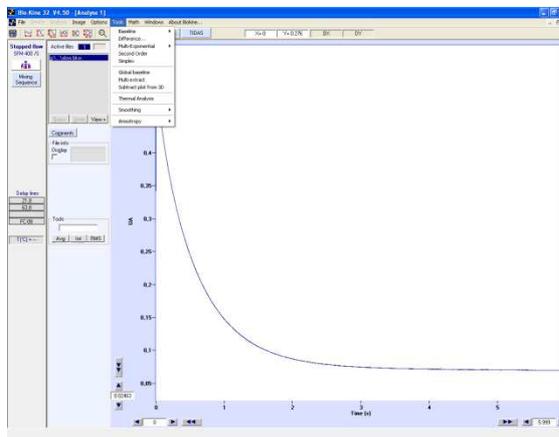

## Specifications

| Light source              |   |
|---------------------------|---|
| Number of lamps           | 2   |
| Nature/Power              | super quiet 150W Xe(Hg) <b>and</b> 150W Xe<br>(tungsten lamp available in option) |
| Wavelength range          | 220 to 700 nm Xe(Hg)<br>200 to 800 nm Xe  |
| Stability                 | better than 1% for Xe(Hg)<br>better than 0,3% for Xe                              |
| Nature of spectrum        | sharp lines for Xe(Hg)<br>continuous spectrum for Xe                              |
| Light source power supply |   |
| Ripple ( 50 to 60Hz)      | < 0,1 % rms   |
| Low frequency noise       | < 0,05 % peak to peak   |
| Drift                     | < 0,1% minute after one hour warm up  |
| Motorized Monochromator   |   |
| Grating                   | 1200 grooves/ nm  |
| Focal length              | 100 mm  |
| Aperture                  | F/# = 3,5   |
| Wavelength range          | zero order and 200-800 nm   |
| Linear dispersion         | 8 nm/mm   |
| Accuracy                  | ± 0,5 nm  |

Specifications are subject to change without prior notice

| Fiber optic                 |   |
|-----------------------------|---|
| Material                    | quartz  |
| Wavelength range            | 200-800 nm  |
| Length                      | 1,5 m   |
| Dimensions                  | 1mm x 3mm ( monochromator side)<br>1,9 mm diameter ( stopped-flow side) |
| Detection                   |   |
| Photomultiplier tube        | 11 stage, optimized for UV <b>and</b> visible                           |
| Operating voltage           | 0 to 1200 V   |
| Wavelength range            | 160 to 850 nm   |
| Low-pass filters            | automatic   |
| Data acquisition            |   |
| Acquisition board type      | High speed 4 channel A/D  |
| Sampling rate               | 10 µs to 1000s/ point   |
| Number of time bases        | 1 to 3  |
| Noise level in fluorescence | S/N > 1000 at 1 ms integration time<br>(using FC-15 and 1µM NATA)       |
| Noise level in absorbance   | 5x10 <sup>-5</sup> AU rms at 1ms integration time                       |
| System requirements         | Windows PC with 2000, XP, Vista and<br>1 open PCI slot (required)       |

### Included with MOS-200/M

- ◆ Optical rail
- ◆ Motorized monochromator
- ◆ Photomultiplier tube
- ◆ Photomultiplier control unit (PMS-250)
- ◆ Acquisition board and communication cable
- ◆ 320 nm cut-off filter
- ◆ Double light source + power supply (ALX-250)
- ◆ 1.5 meter fiber optics (other dimensions available on request)
- ◆ Fiber optics adaptor for stopped-flow head
- ◆ Trigger cable
- ◆ Bio-Kine and SFit software
- ◆ MM-450 control unit

## Endless upgrade possibilities

### T-format anisotropy kit :

It includes a set of Glan-Taylor polarizers and an additional detection channel. Polarizers are installed in PMT holder for easy removal in absorbance mode. Triple simultaneous measurements (absorbance/T-format anisotropy, fluorescence) is available with optional 049-10.

### Additional detection channel :

For simultaneous absorbance/fluorescence and double fluorescence measurements. This includes a second photomultiplier tube and control unit.

### MOS-450/AF-CD :

MOS-200/M can be upgraded to more advanced spectrometer models with detection techniques such as Circular Dichroism, Linear dichroism and Fluorescence Anisotropy using **our patented EMFA method (Excitation Modulated Fluorescence Anisotropy)**.

### Emission monochromator:

For fluorescence emission spectra or kinetics detection at a fixed wavelength. Monochromator is available in both manual and motorized version.

Bio-Logic, SAS  
1, rue de l'Europe  
38640 CLAIIX - France  
Tel.: +33 476 98 68 31  
Fax: +33 476 98 69 09  
www.bio-logic.info



Bio-Logic USA, LLC  
P.O.Box 30009  
Knoxville TN 37930 - USA  
Tel.: +1 865 769 3800  
Fax: +1 865 769 3801  
Web: www.bio-logic.us